



Certificate of Analysis




Material	Lot	Batch	Expiration date*
Chromosorb 108	13031	14505	April, 2025

* This expiration date is for sealed tubes. Tubes that are open-ended and made from this batch will have a shorter shelf life.

This batch of sorbent has met our QC requirements as outlined in SKC Procedure 4052.

Scott Marshall
QA Manager

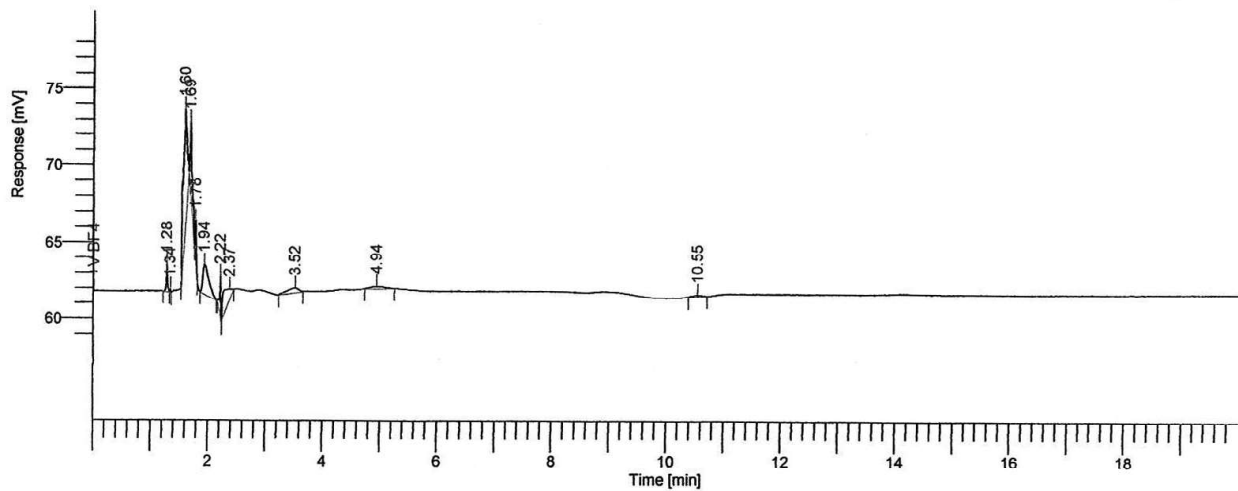

All peaks less than 5 $\mu\text{g/g}$ calculated as Naphthalene.